

# InertSustainBio C18

## *Rapid Separations of Proteins and Peptides*

### High Recoveries of Proteins and Peptides

The 200 Å pore size silica creates the opportunity to separate compounds having a molecular weight from small to large molecules. In addition, the usage of highly inert packing material packed into a new Steel-Coated-PEEK hardware deliver excellent peak shapes for various analytes without any adsorption.

### Physical Properties

Silica :	ES (Evolved Surface) Silica Gel
Particle Size :	1.9 µm, 3 µm
Surface Area :	200 m <sup>2</sup> /g
Pore Size :	200 Å (20 nm)
Pore Volume :	1.00 mL/g
Bonded Phase :	Octadecyl Groups
End-capping :	Complete
Carbon Loading :	9.0 %
USP Code :	L1
pH Range :	1.0 to 10.0
Max. Operating Pressure:	80 MPa, 800 Bar for 1.9 µm columns 50 MPa, 500 Bar for 3 µm columns




### Benefits

- Separation of compounds from small to large molecules
- A radically new Steel-Coated-PEEK hardware preventing adsorption of peaks
- Suitable for analyzing Phosphate compounds WITHOUT the formation of phosphate-iron complexes found with stainless steel column hardware
- Extreme resistance to low and high pH mobile phases
- Endlessly reproducible from column-to-column and batch-to-batch for consistent results

# InertSustainBio C18 HPLC Columns

## Effects of Pore Size

The molecular weight of peptides and oligonucleotides are from several kDa to several dozen kDa. It is critically important to select the appropriate pore size column to achieve high efficiency. As shown below, the optimized 200 Å pore size silica enables InertSustainBio C18 to analyze peptides and oligonucleotides.



## Analysis of Proteins

### Conditions

Column : InertSustainBio C18 (1.9 µm, 50 x 2.1 mm I.D.)

Eluent : A) 0.1 % HCOOH in H<sub>2</sub>O

B) 0.1 % HCOOH in CH<sub>3</sub>CN

A/B = 80/20 - (2.5 min) - 20/80 - (0.5 min) - 20/80, v/v


Flow Rate : 0.5 mL/min

Col. Temp. : 40 °C

Detection : UV 280 nm

Injection Vol. : 5 µL

Sample : Proteins (100 mg/mL each)




## A Radically New Steel-Coated-PEEK Hardware

Generally, conventional PEEK hardware is tolerable up to a back pressure of 20 MPa. The mechanical strength of PEEK is far less than stainless steel and the durability to be very low as well. As illustrated below, the introduction of a radically new Steel-Coated-PEEK hardware in InertSustainBio C18 offer maximum operating pressure of 80 MPa for 1.9  $\mu\text{m}$  columns achieving rapid analysis for analytes sensitive to frequently used stainless steel columns.

### Comparison of Hardware Structure


#### InertSustainBio C18

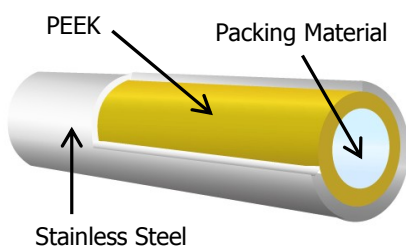

- Max. Operating Pressure: 80 MPa

- PEEK frit


#### Conventional PEEK Hardware



- Max. Operating Pressure: 20 MPa

- PEEK frit

#### Stainless Steel Hardware



- Max. Operating Pressure: 80 MPa

- Sintered metal frit




Access to the latest pharmaceutical, life science, environmental and food applications at [www.glsciences.com/tech/inertsearch](http://www.glsciences.com/tech/inertsearch)

# InertSustainBio C18 HPLC Columns

## Analysis of Coenzyme A

As shown in the following chemical structure, Coenzyme A have several phosphate groups which is a sample sensitive to stainless steel hardware. InertSustainBio C18 successfully eluted Coenzyme A without any adsorption while stainless steel columns failed.



### Conditions

Column : InertSustainBio C18 (1.9  $\mu$ m, 50 x 2.1 mm I.D.)

Eluent : A) 5 mM HCOONH<sub>4</sub> in H<sub>2</sub>O

B) 5 mM HCOONH<sub>4</sub> in CH<sub>3</sub>CN

A/B = 98/2 - (2 min) - 80/20 - (0.01 min) -  
98/2 - (2.99 min) - 98/2, v/v

Flow Rate : 0.4 mL/min

Col. Temp. : 40 °C


Detection : MS/MS (ESI positive)

Injection Vol. : 10  $\mu$ L


Sample : Coenzyme A 500 ng/mL

Q1/Q3: 768.05/261.0

### InertSustainBio C18

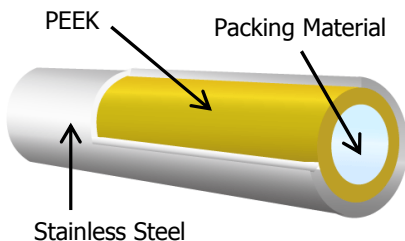


■ Pore Size 200 Å, 1.9  $\mu$ m



### Stainless Steel Hardware Packed with InertSustainBio C18




■ Pore Size 200 Å, 1.9  $\mu$ m




### Stainless Steel Hardware Acquity BEH C18



■ Pore Size 130 Å, 1.7  $\mu$ m




## Analysis of Oligonucleotides

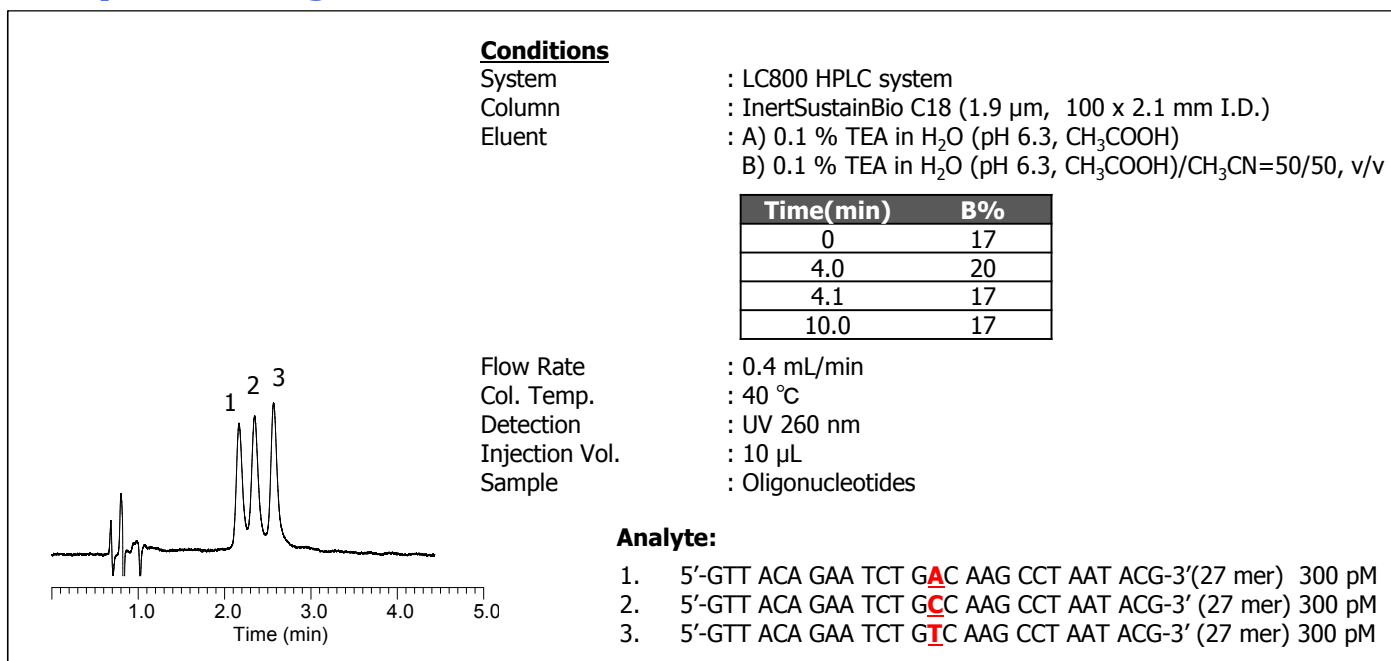

## Analysis of Peptides

A batch test report made by analysis of standard peptides is attached to every column assuring great reproducibility from column-to-column and batch-to-batch for consistent results.

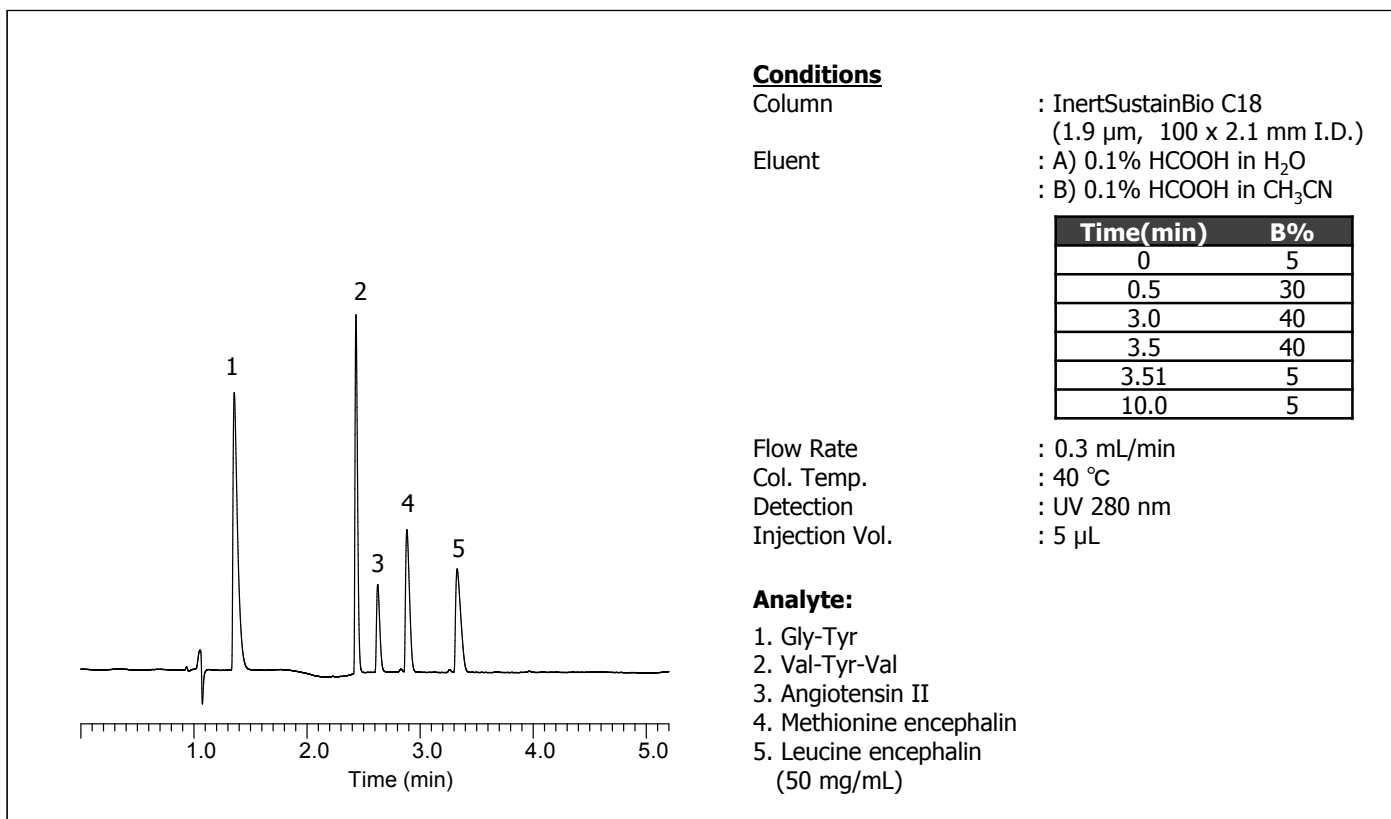


## InertSustainBio C18 HPLC Columns

### Analytical Columns

Cat#	Description	Max. Operating Pressure (MPa)
5020-89500	InertSustainBio C18 1.9 $\mu$ m 2.1x50mm	80
5020-89501	InertSustainBio C18 1.9 $\mu$ m 2.1x100mm	80
5020-89502	InertSustainBio C18 1.9 $\mu$ m 2.1x150mm	80
5020-89503	InertSustainBio C18 HP 3 $\mu$ m 2.1x50mm	50
5020-89504	InertSustainBio C18 HP 3 $\mu$ m 2.1x100mm	50
5020-89505	InertSustainBio C18 HP 3 $\mu$ m 2.1x150mm	50

\* As shown below, end-fittings are "UP" type end-fittings, which are UHPLC compatible end-fittings for UHPLC systems (Ex: UPLC®) to avoid dead volume.

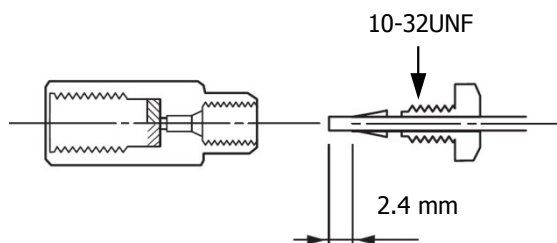

UPLC® is a registered trademark of Waters Corporation.

## Worldwide Ordering Information

### GL Sciences, Inc. USA

4733 Torrance Blvd. Suite 255  
Torrance, CA 90503  
Phone: 310-265-4424  
Fax: 310-265-4425  
Email: [info@glsciencesinc.com](mailto:info@glsciencesinc.com)  
Web: [www.glsciencesinc.com](http://www.glsciencesinc.com)

### GL Sciences B.V.

De Sleutel 9  
5652 AS Eindhoven  
The Netherlands  
Phone: +31 (0)40 254 95 31  
Fax: +31 (0)40 254 97 79  
Email: [info@glsciences.eu](mailto:info@glsciences.eu)  
Web: [www.glsciences.eu](http://www.glsciences.eu)

### International Distributors

Visit our Website at  
[www.glsciences.com/distributors](http://www.glsciences.com/distributors)

### GL Sciences, Inc. Japan

22-1 Nishishinjuku 6-Chome  
Shinjuku-ku, Tokyo,  
163-1130, Japan  
Phone: +81-3-5323-6620  
Fax: +81-3-5323-6621  
Email: [world@glsc.co.jp](mailto:world@glsc.co.jp)  
Web: [www.glsciences.com](http://www.glsciences.com)

The GL Sciences name, the GL Sciences logo are the property of GL Sciences Inc.

All other trademarks or service marks are the property of their respective owners.

The specification and the column type are subject to change without notice due to continual improvements.

**GL Sciences Inc.**